

APPENDIX F

I/O DATA FOR PDU-10 FLUID DYNAMIC TESTS

FIGURE F -- 1
**PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 01**

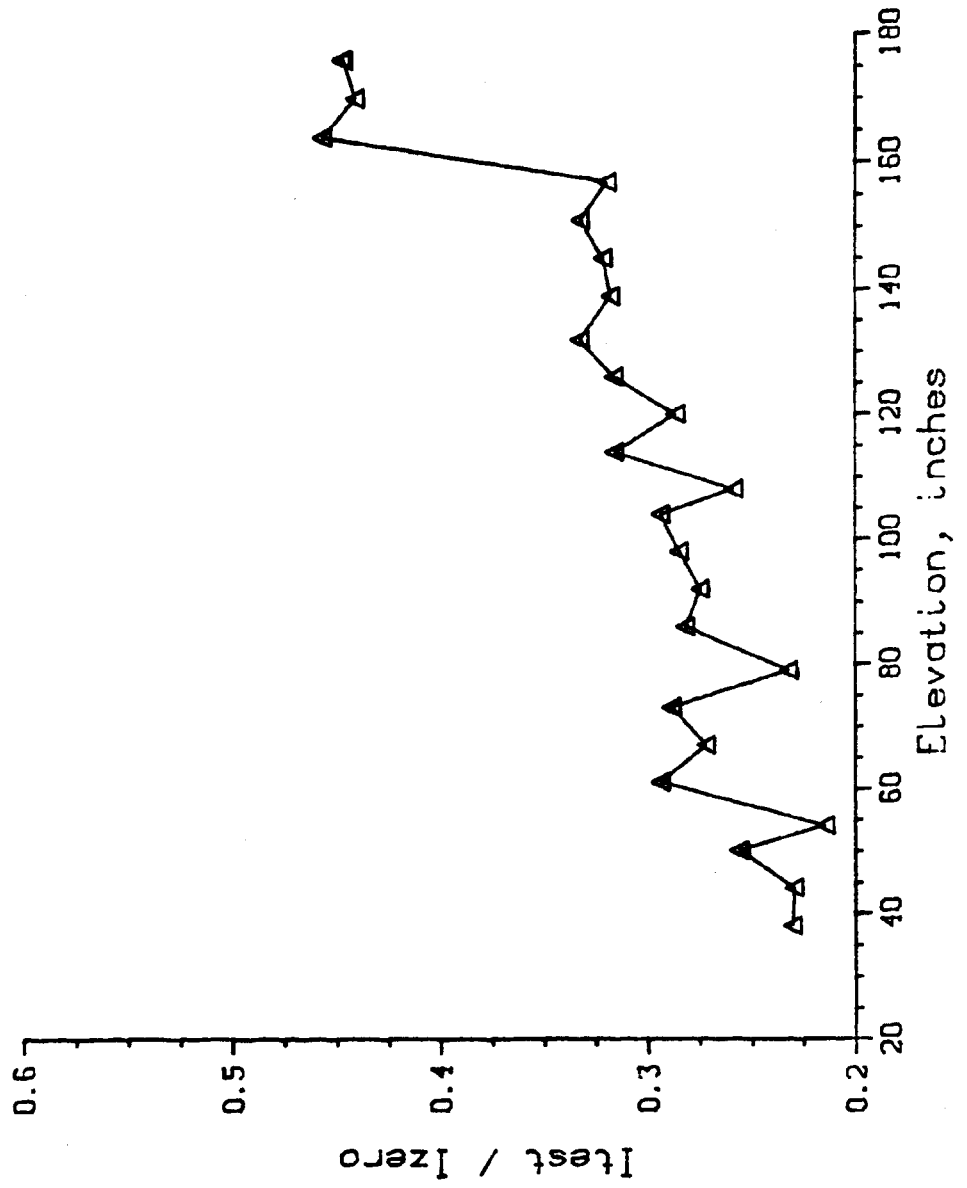


FIGURE F - 2
**PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 02**

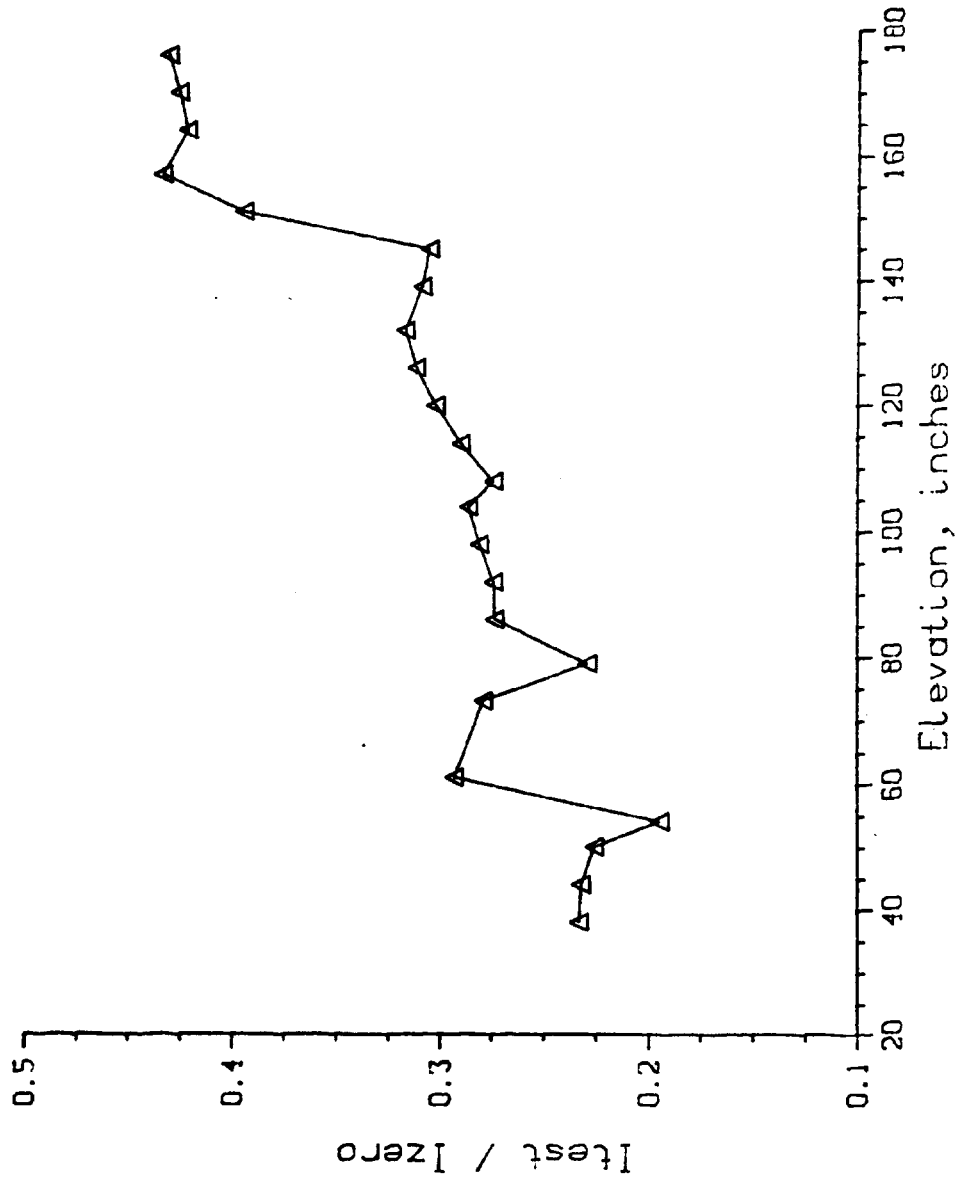


FIGURE F - 3
**PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 03**

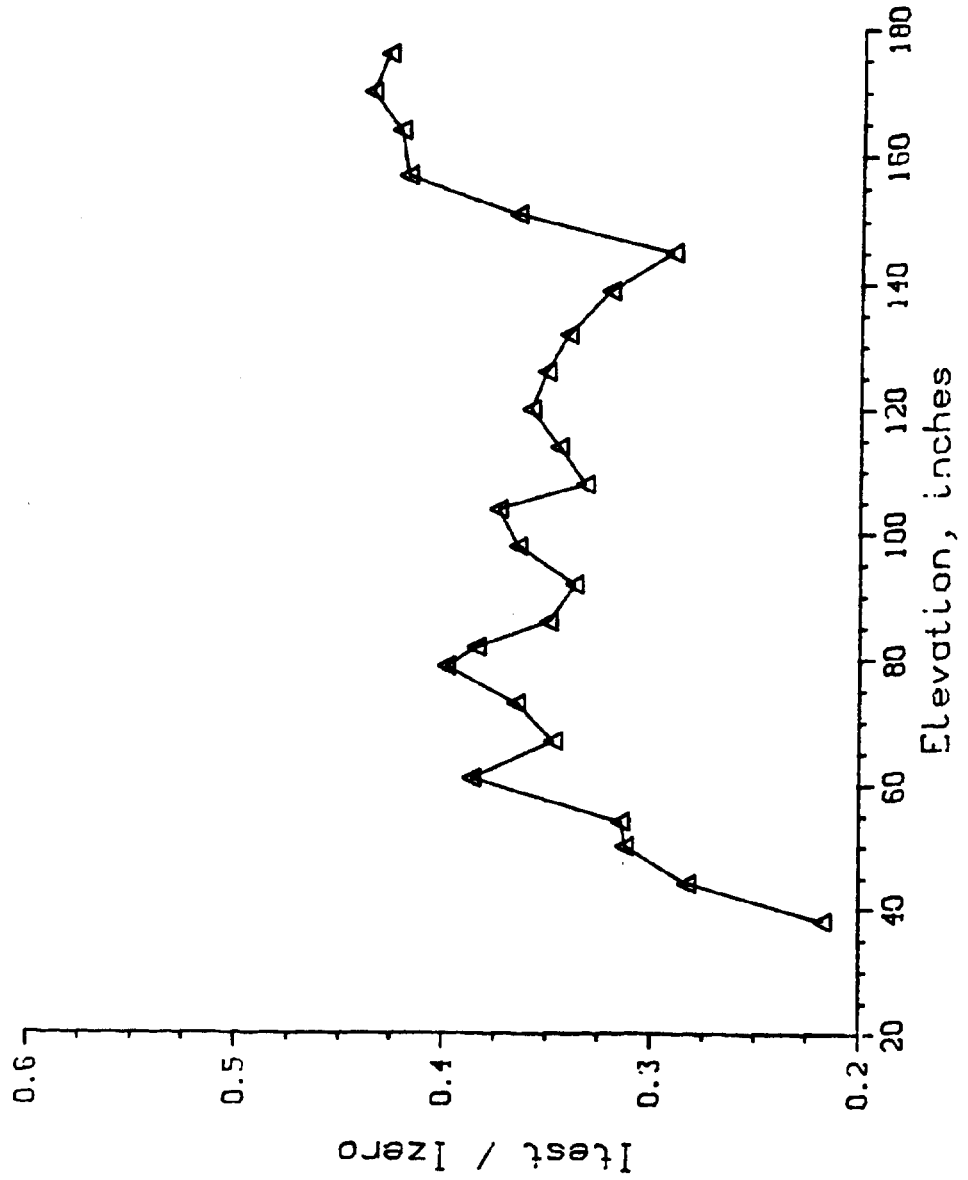


FIGURE F -- 4
**PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 04**

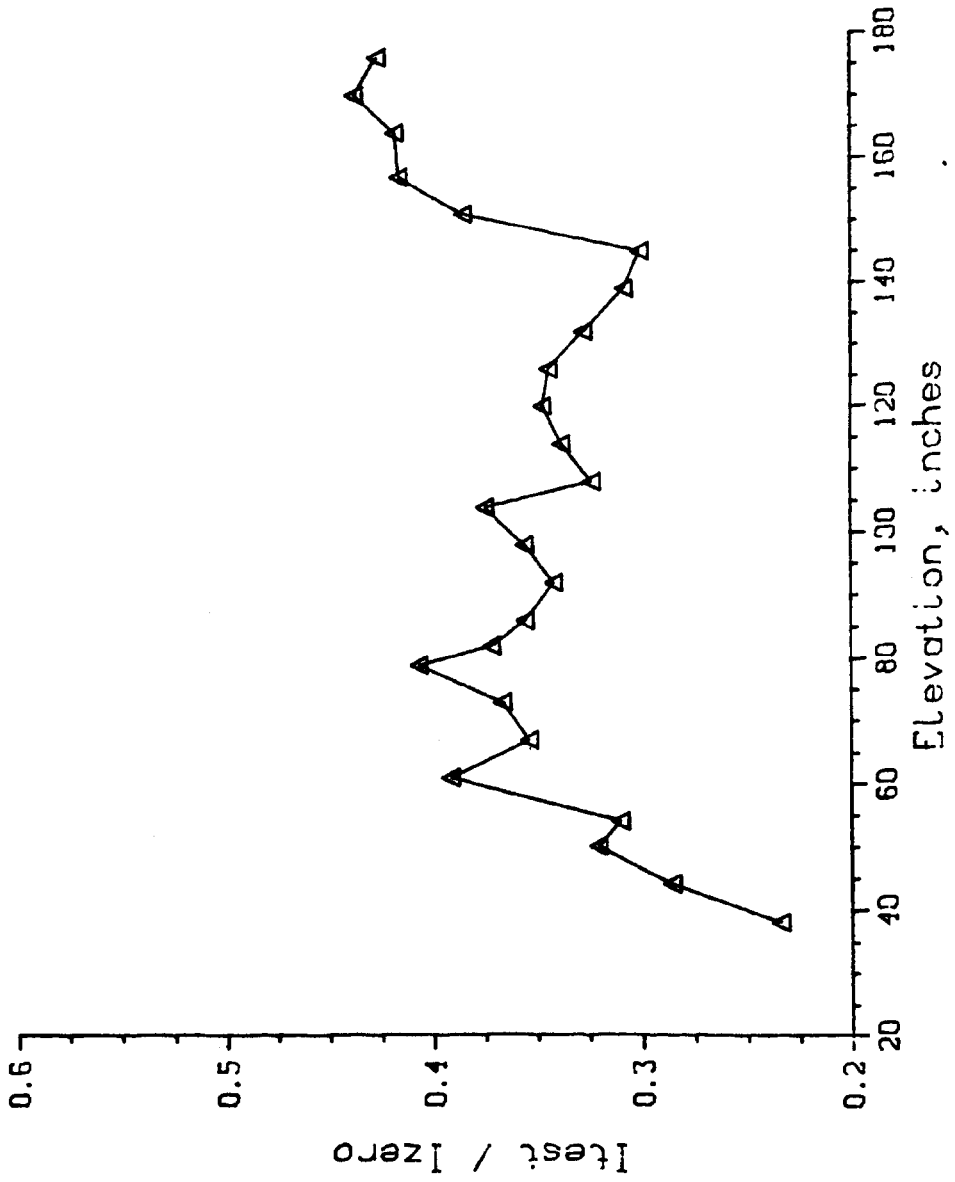


FIGURE F - 5
**PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 05**

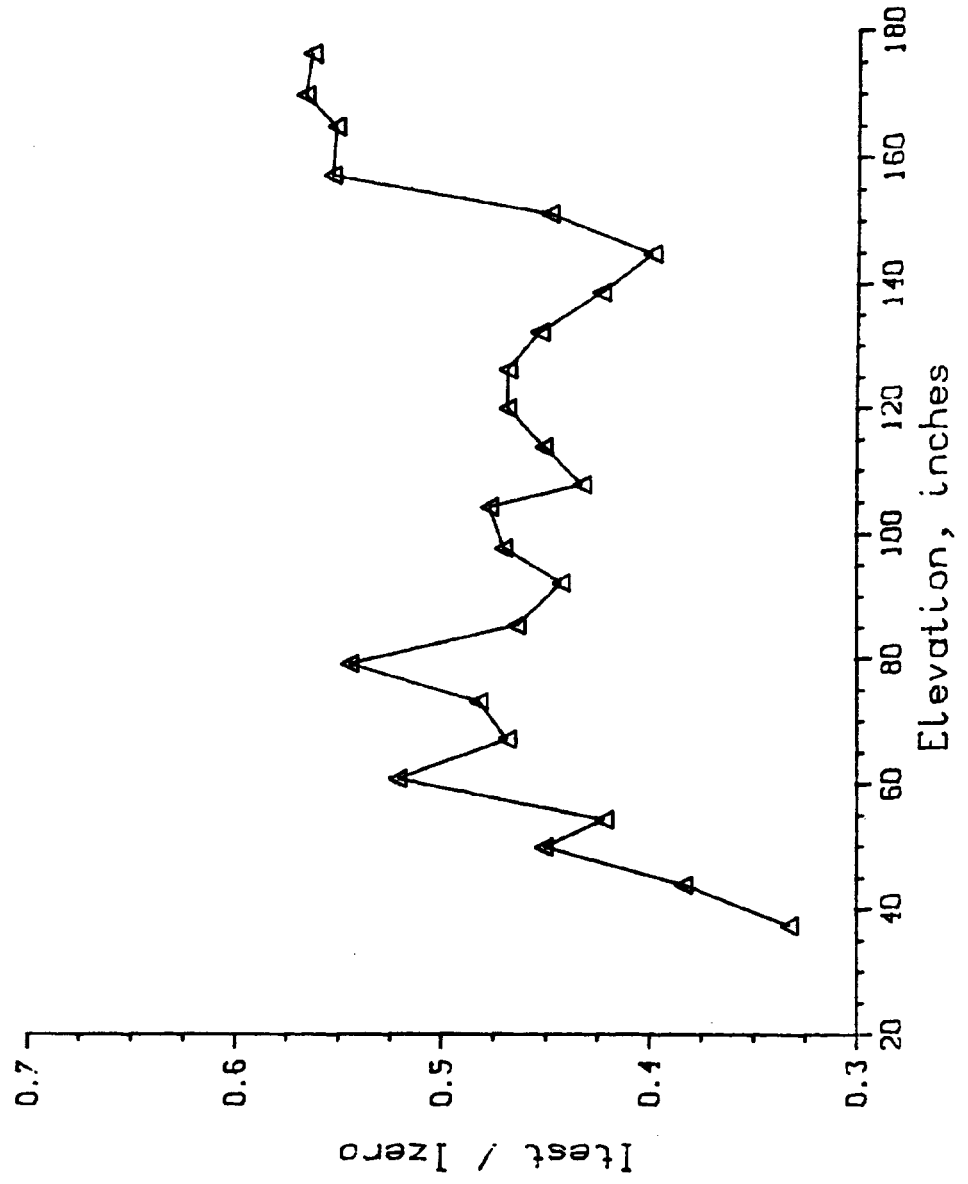


FIGURE F - 6
**PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 06**

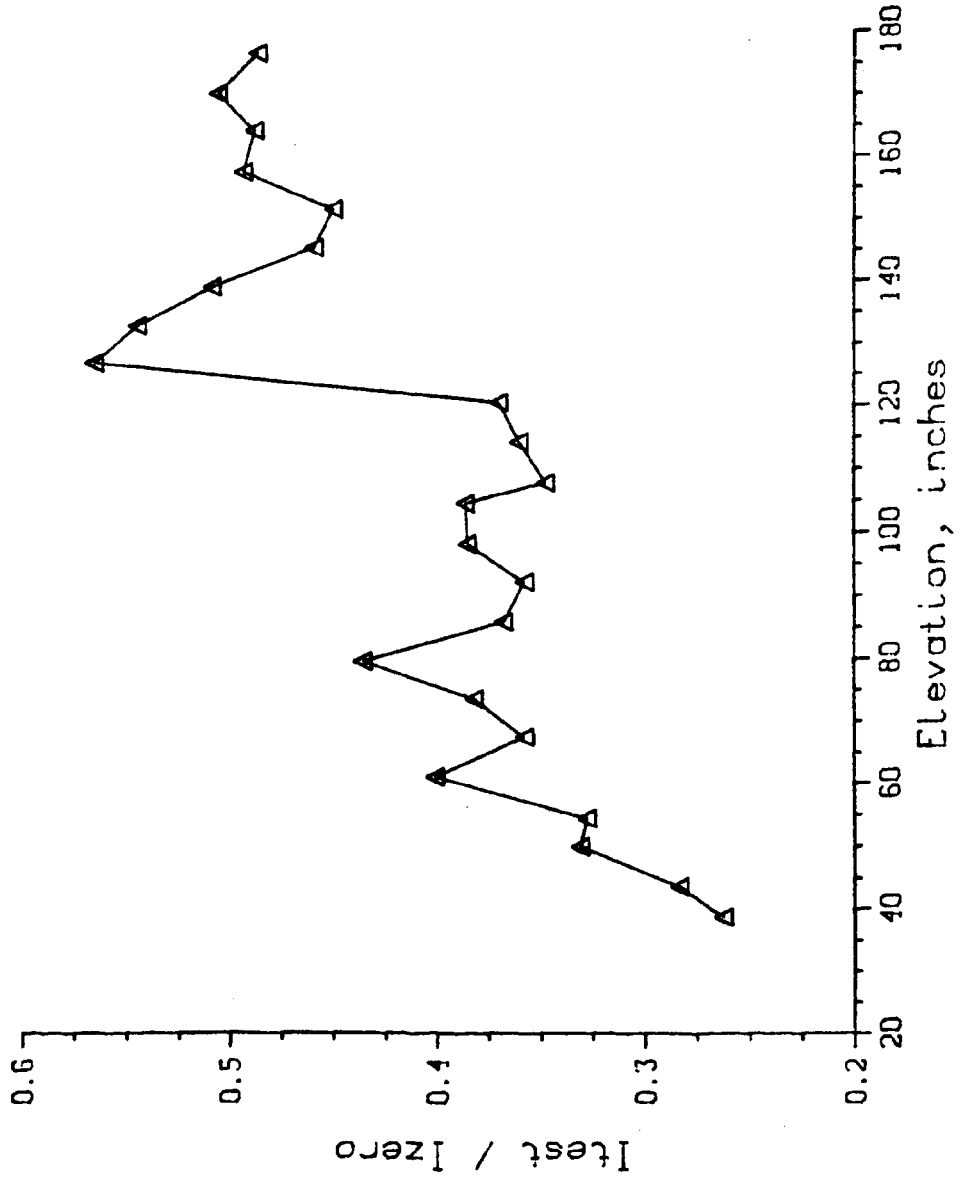


FIGURE F - 7
**PDU-10 GAMMA RAY SCAN
I/I0 RATIO, TEST NUMBER 07**

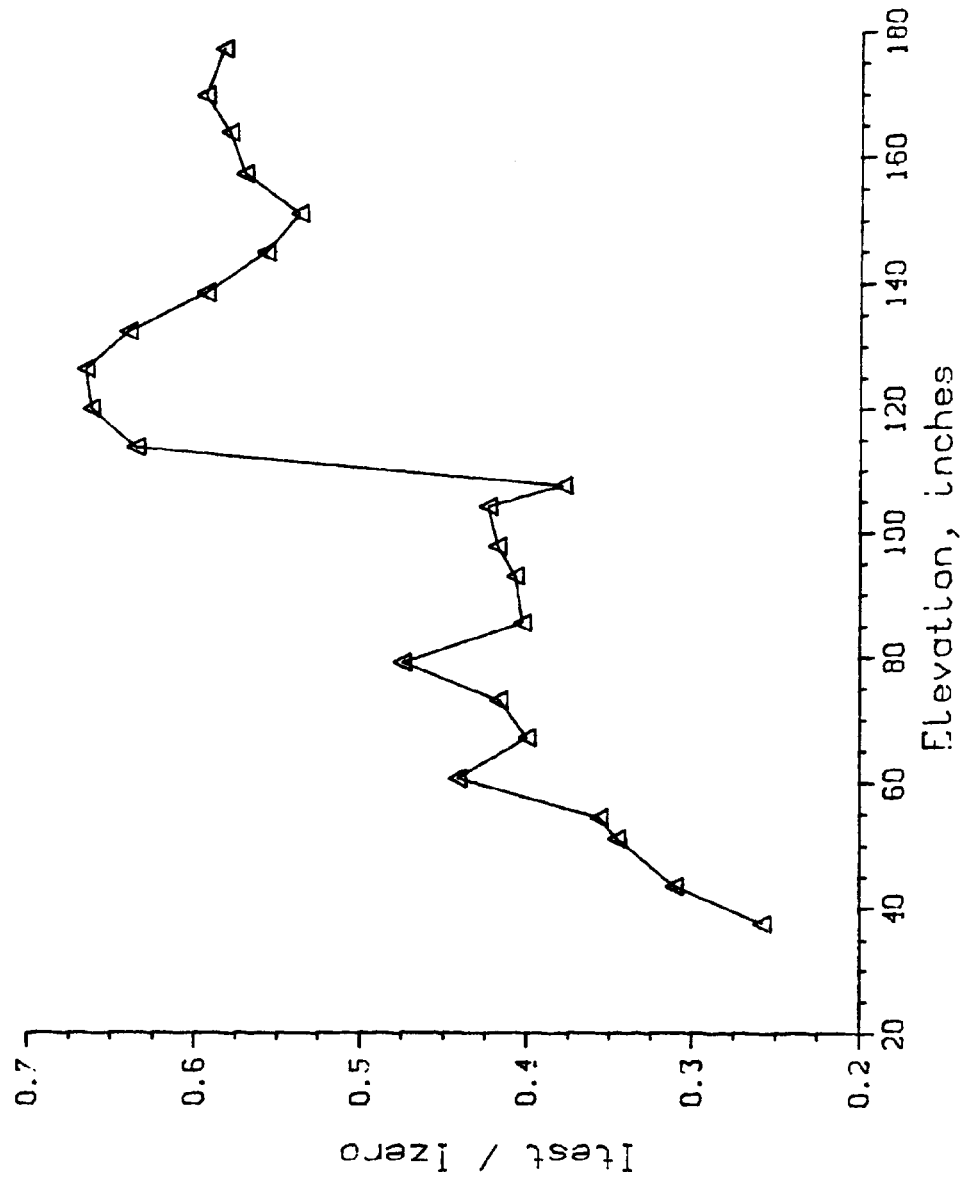


FIGURE F -- 8

**PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 08**

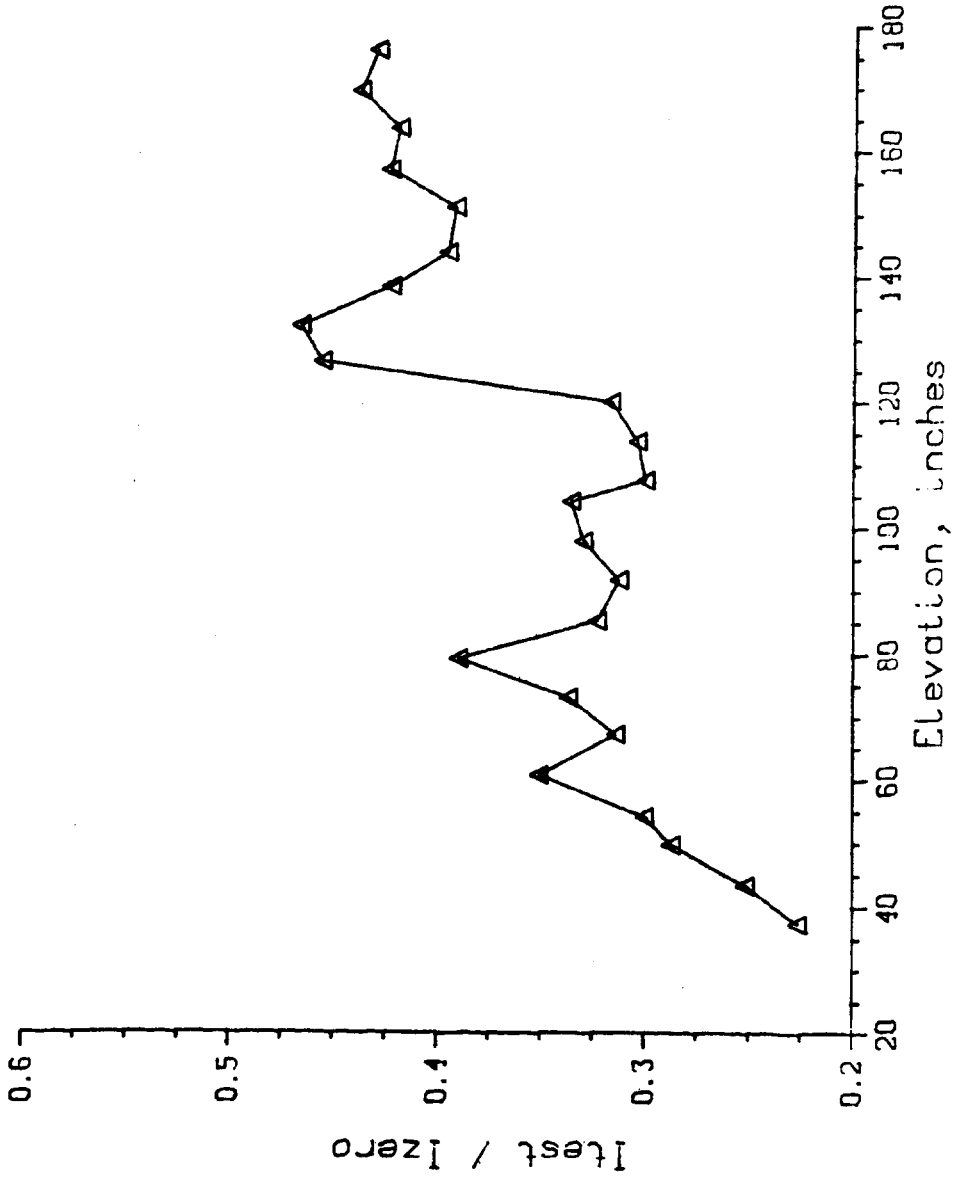


FIGURE F - 9
PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 09

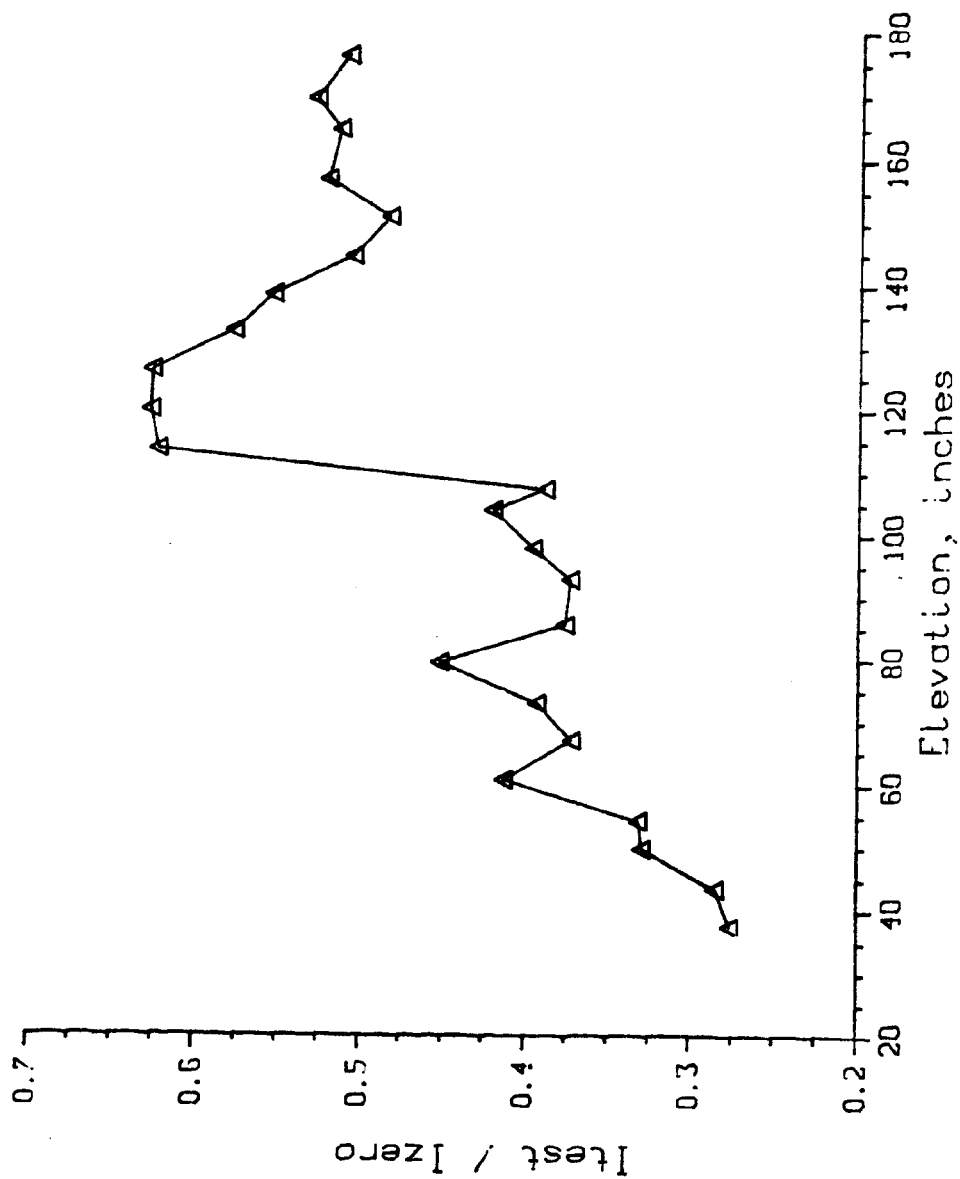


FIGURE F -10
**PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 10**

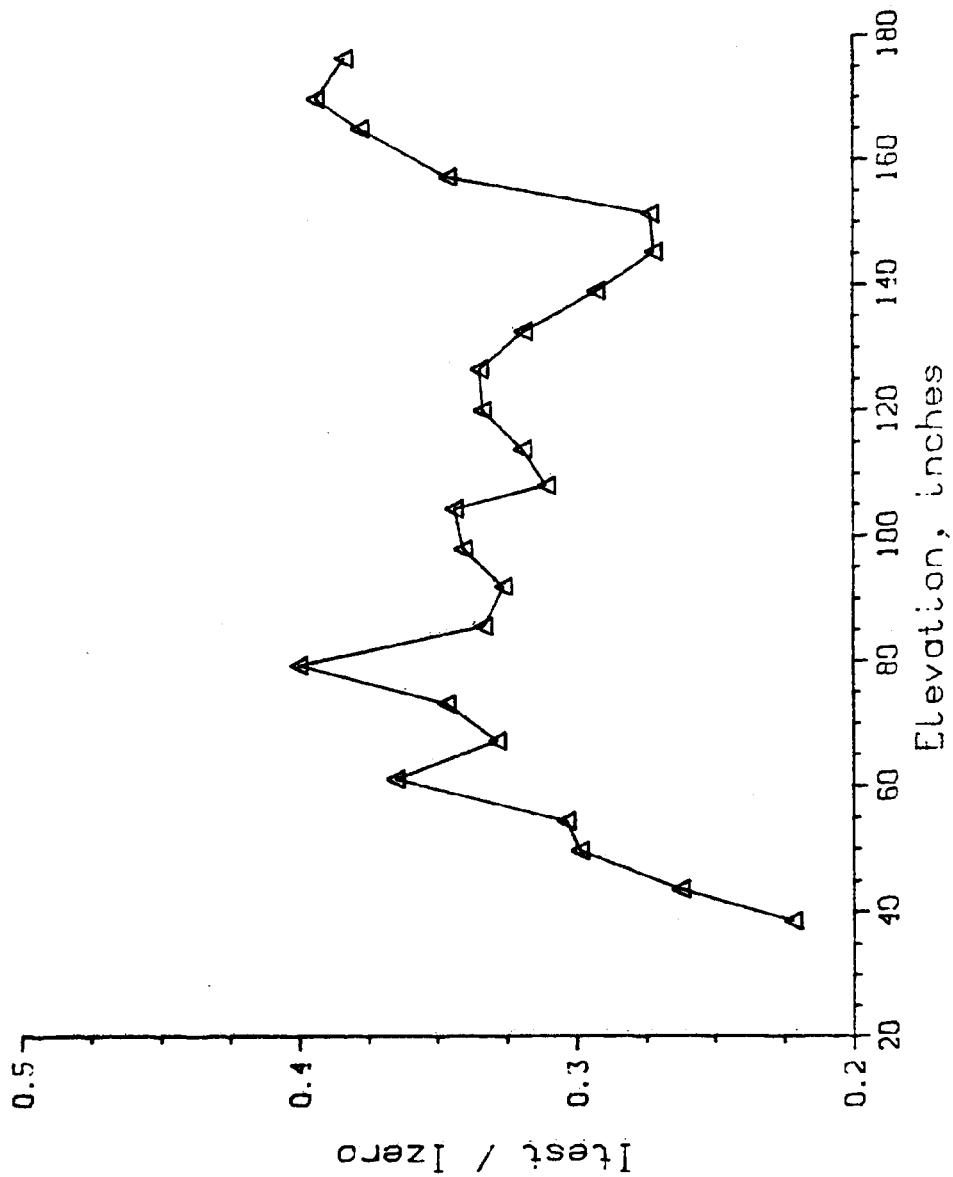


FIGURE F -11
**PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 11**

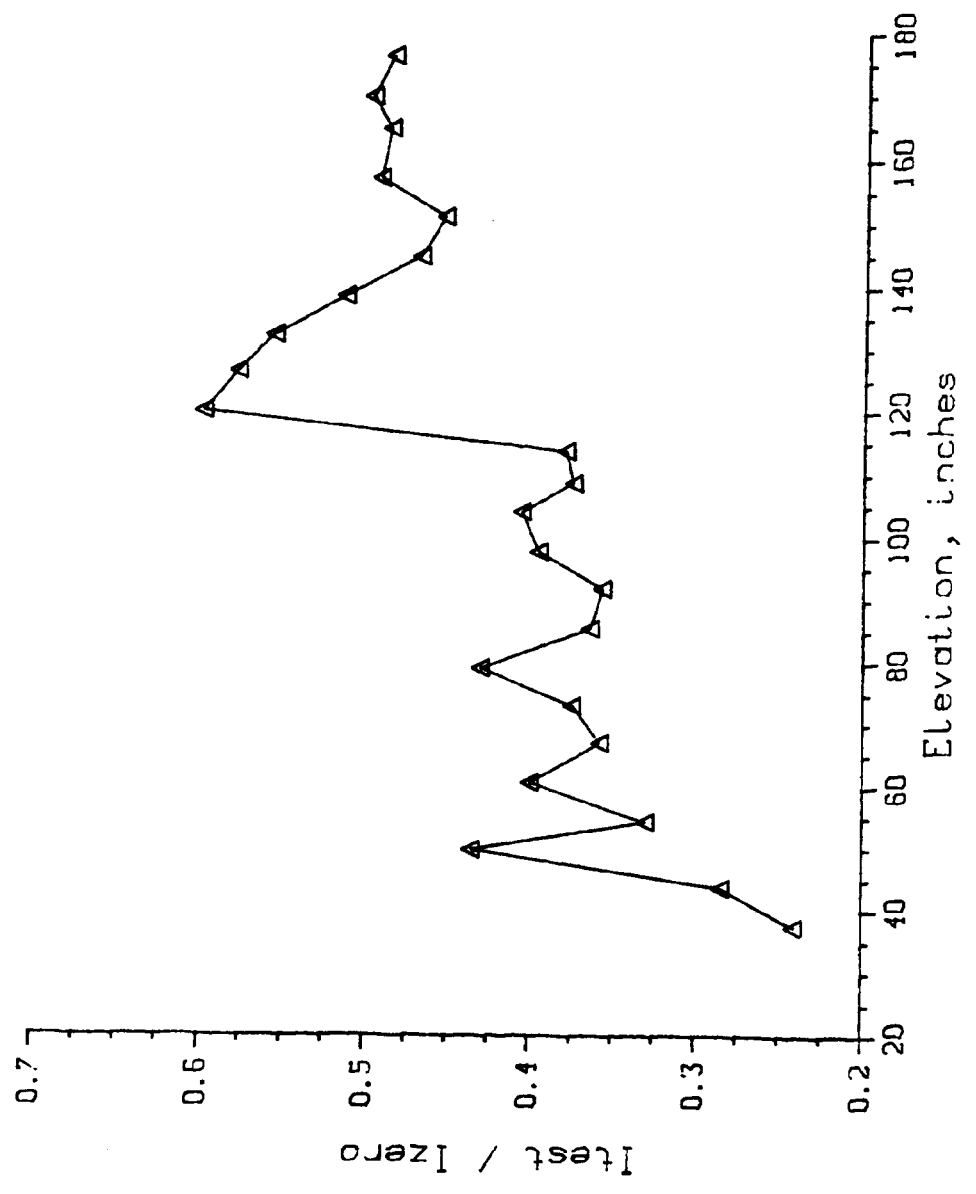


FIGURE F --12
**PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 12**

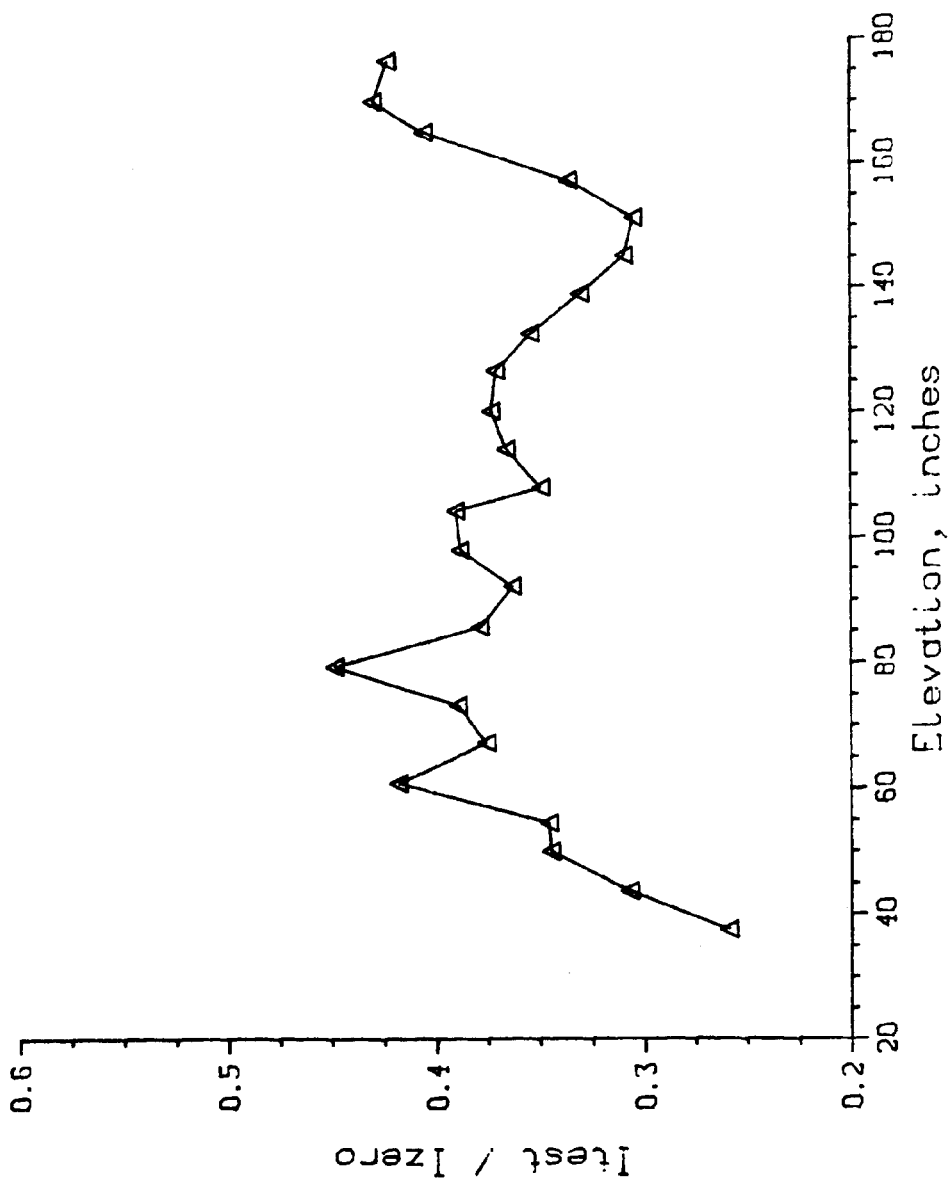


FIGURE F -13
PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 13

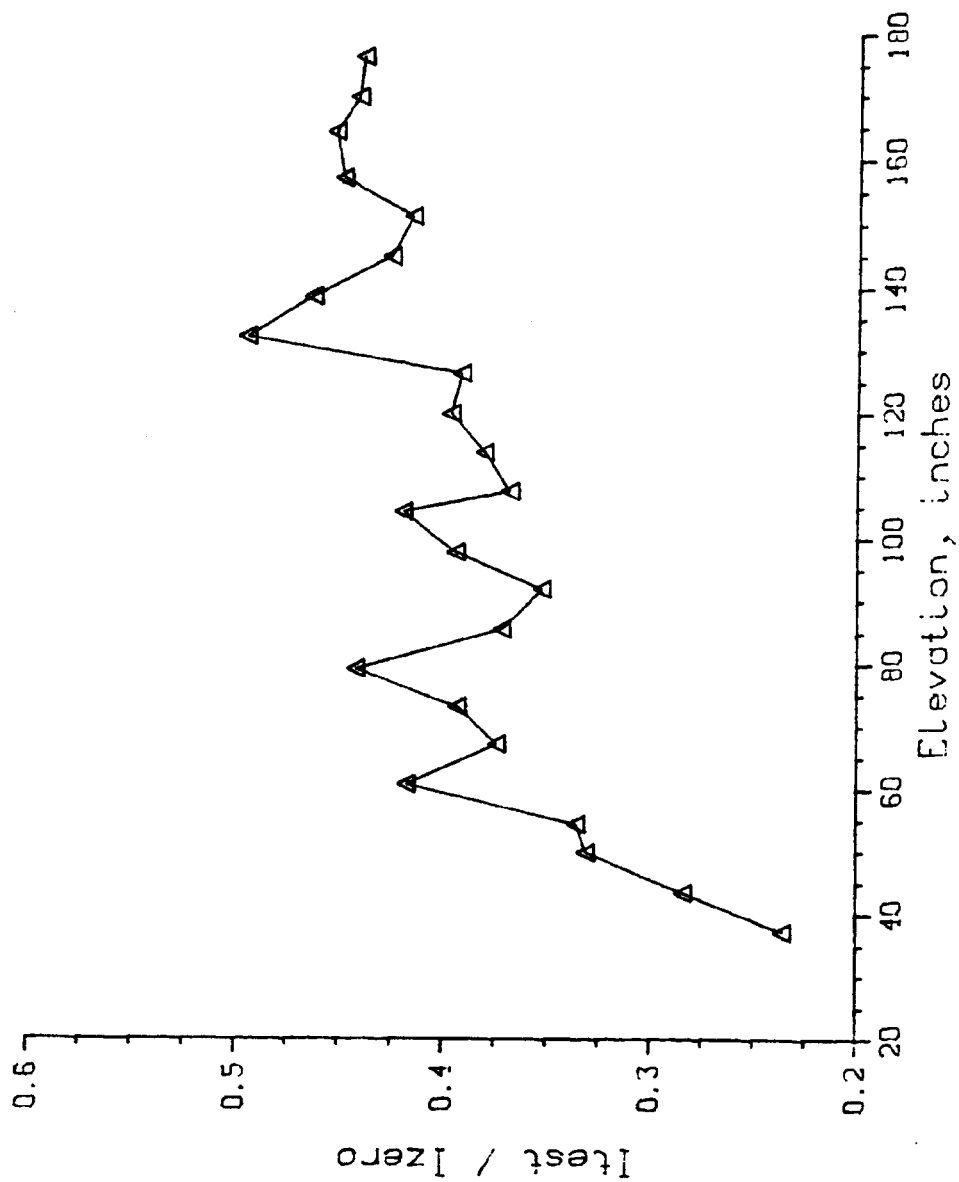


FIGURE F -14
**PDU-10 GAMMA RAY SCAN
I/I0 RATIO, TEST NUMBER 14.**

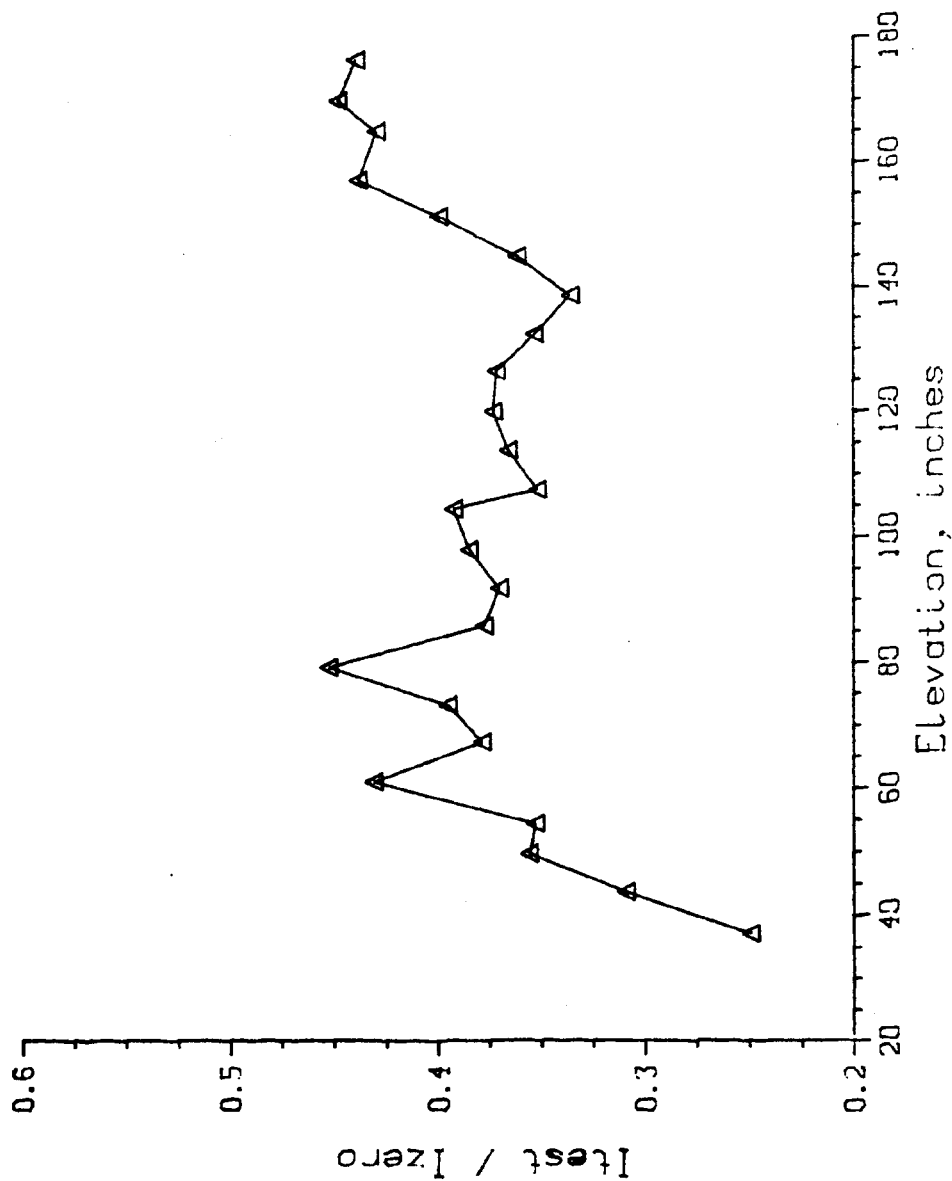


FIGURE F -15
**PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 15**

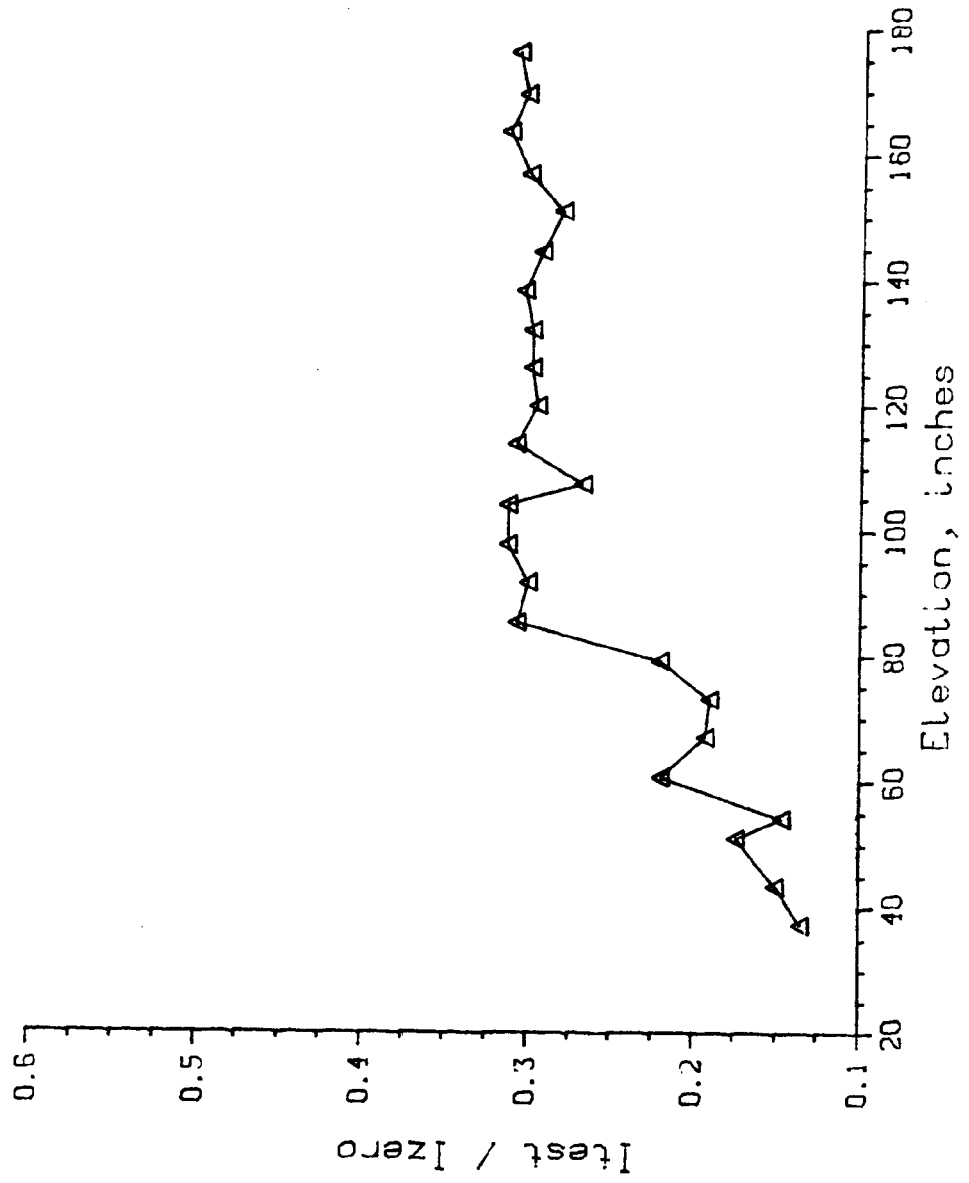


FIGURE F -16
**PDU-10 GAMMA RAY SCAN
I/10 RATIO, TEST NUMBER 16**

